

Worry-Free® Pull-Cord Alarm, #72140

Instructions for Use and Care

Description


Your new AliMed® Worry-Free Pull-Cord Alarm alerts caregivers when a patient attempts to exit a wheelchair or bed without assistance. A tug on the cord from any direction will dislodge the magnetic sensor and activate the alarm. Alarm attaches to a wheelchair or bed.

Use

- Attach to wheelchair or bed with pinch-clip on back of alarm (Figure 1).
- On/Off switch is hidden under sensor cover. Slide switch to “ON” position and place magnetic sensor in sensor area on alarm (Figure 2).
- Secure cord to patient using alligator clip. Attach to clothing they are not likely to remove. Locate clip out of patient’s reach. Using cord adjuster, adjust length of cord to ensure it does not entangle or choke patient (Figure 3).
- A tug on the cord in any direction will cause magnetic sensor to release and alarm will be triggered. Stop alarm by replacing sensor or turning unit off.

Battery information

This alarm is intended as a single-use alarm and is equipped with a long-life battery that should provide approximately 30 days of use. Unit is guaranteed for 30 days and is intended for disposal at battery depletion.

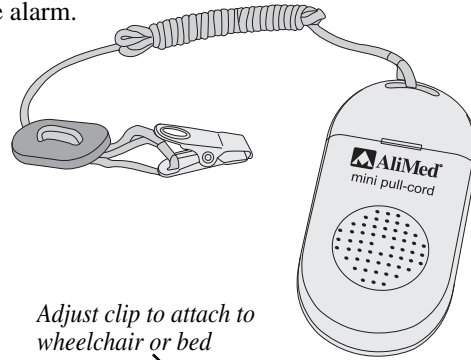

Adjust clip to attach to wheelchair or bed

Figure 1


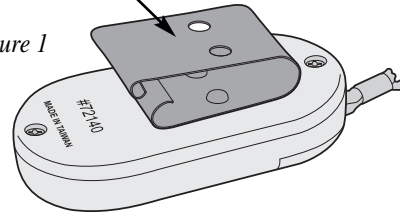


Figure 2



Figure 3

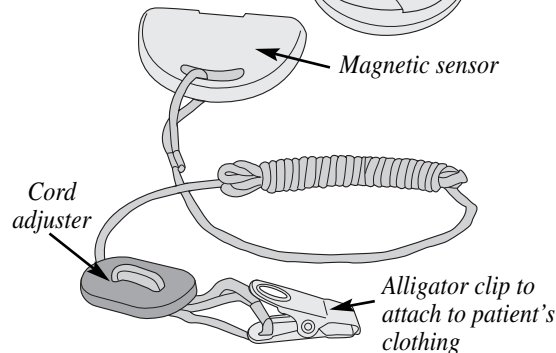

Manufactured for:



AliMed® inc.

297 High St., Dedham, MA 02026 USA
PH 800.225.2610 • FAX 800.437.2966

AliMed.com
#5548REV0216 CCO818
©2016 AliMed® inc. All rights reserved.
Made in Taiwan

Worry-Free® Pull-Cord Alarm, #72140

Instructions for Use and Care

Description


Your new AliMed® Worry-Free Pull-Cord Alarm alerts caregivers when a patient attempts to exit a wheelchair or bed without assistance. A tug on the cord from any direction will dislodge the magnetic sensor and activate the alarm. Alarm attaches to a wheelchair or bed.

Use

- Attach to wheelchair or bed with pinch-clip on back of alarm (Figure 1).
- On/Off switch is hidden under sensor cover. Slide switch to “ON” position and place magnetic sensor in sensor area on alarm (Figure 2).
- Secure cord to patient using alligator clip. Attach to clothing they are not likely to remove. Locate clip out of patient’s reach. Using cord adjuster, adjust length of cord to ensure it does not entangle or choke patient (Figure 3).
- A tug on the cord in any direction will cause magnetic sensor to release and alarm will be triggered. Stop alarm by replacing sensor or turning unit off.

Battery information

This alarm is intended as a single-use alarm and is equipped with a long-life battery that should provide approximately 30 days of use. Unit is guaranteed for 30 days and is intended for disposal at battery depletion.

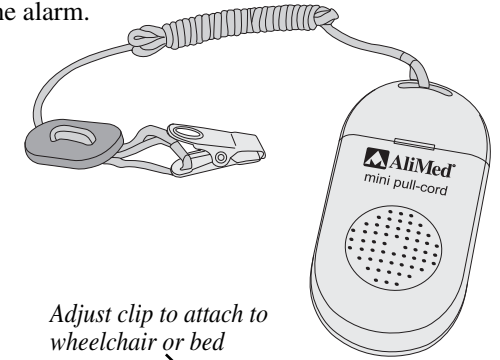

Adjust clip to attach to wheelchair or bed

Figure 1


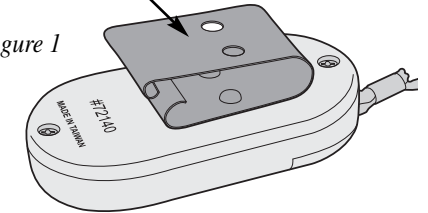


Figure 2



Figure 3

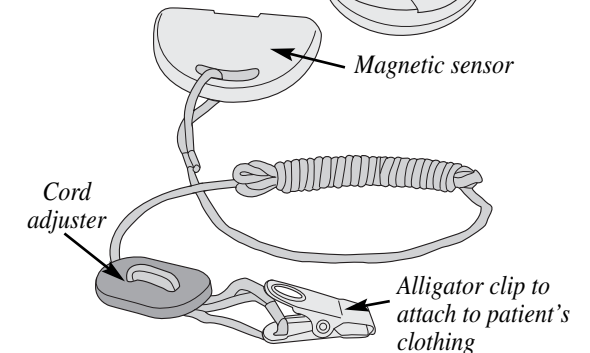

Manufactured for:



AliMed® inc.

297 High St., Dedham, MA 02026 USA
PH 800.225.2610 • FAX 800.437.2966

AliMed.com
#5548REV0216 CCO818
©2016 AliMed® inc. All rights reserved.
Made in Taiwan

Care

- Wipe clean using standard disinfectants.
- Suggested cleaning agent: SaniGuard® Dry-on-Contact Sanitizing Surface Spray (#7266812, 12/cs), an EPA-registered sanitizer that kills 99.9% of all germs, bacteria, and viruses on contact. Dries on contact.
- Do not immerse in fluids.
- Check function before each use.

Caution:

This device is not a substitute for routine visual monitoring of patients. It will not prevent falls. Staff must make frequent inspections to ensure alarm unit is functioning properly. Long pull-cord can entangle patient and is potentially dangerous if not adjusted correctly.

Construction

ABS plastic, magnet

Reorder Information

- #72140 Worry-Free Pull-Cord Alarm
 - #7214010 Worry-Free Pull-Cord Alarm, 10/cs
 - #710100 Replacement Pull-Cord, 10/pk
 - #7266812 SaniGuard Dry-on-Contact Sanitizing Surface Spray, 12/cs
-

Care

- Wipe clean using standard disinfectants.
- Suggested cleaning agent: SaniGuard® Dry-on-Contact Sanitizing Surface Spray (#7266812, 12/cs), an EPA-registered sanitizer that kills 99.9% of all germs, bacteria, and viruses on contact. Dries on contact.
- Do not immerse in fluids.
- Check function before each use.

Caution:

This device is not a substitute for routine visual monitoring of patients. It will not prevent falls. Staff must make frequent inspections to ensure alarm unit is functioning properly. Long pull-cord can entangle patient and is potentially dangerous if not adjusted correctly.

Construction

ABS plastic, magnet

Reorder Information

- #72140 Worry-Free Pull-Cord Alarm
 - #7214010 Worry-Free Pull-Cord Alarm, 10/cs
 - #710100 Replacement Pull-Cord, 10/pk
 - #7266812 SaniGuard Dry-on-Contact Sanitizing Surface Spray, 12/cs
-



Manufactured for:



AliMed® inc.

297 High St., Dedham, MA 02026 USA
PH 800.225.2610 • FAX 800.437.2966



MDSS GmbH
Schiffgraben 41
30175 Hannover,
Germany

AliMed.com
#5548REV0216 CCO818
©2016 AliMed® inc. All rights reserved.
Made in Taiwan



Manufactured for:



AliMed® inc.

297 High St., Dedham, MA 02026 USA
PH 800.225.2610 • FAX 800.437.2966



MDSS GmbH
Schiffgraben 41
30175 Hannover,
Germany

AliMed.com
#5548REV0216 CCO818
©2016 AliMed® inc. All rights reserved.
Made in Taiwan