

# AliMed® Tilt Table Strap

## Instructions for Use and Care

### Intended Use

The AliMed® Tilt Table Strap supports a patient during diagnostic or surgical procedures using a tilt table.


### Instructions for Use

*For use by clinician only.*

Reusable.

1. With hook material facing up, place strap over patient and under rail on each side of table (*Figure 1*).
2. Pull ends of straps over patient and toward center of table to desired tension (*Figure 2*).
  - 2.1 To fasten, press hook material firmly into loop surface.

*NOTE: It is recommended to use three straps per patient to provide both practitioner and patient with added level of security and comfort (Figure 3).*

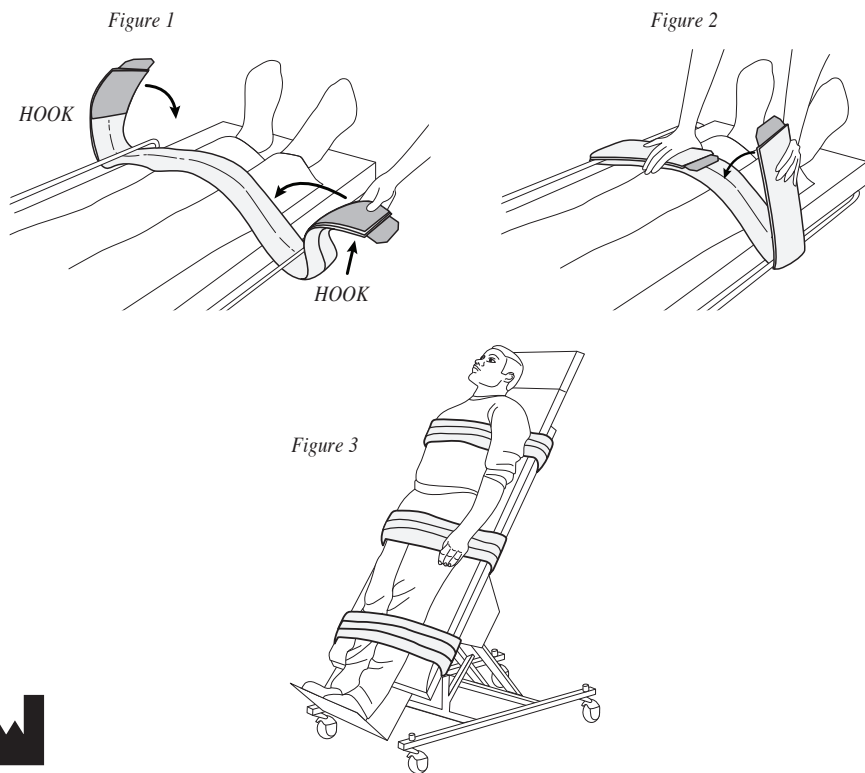

Manufactured for:



**AliMed® Inc.**

297 High St., Dedham, MA 02026 USA  
PH 800.225.2610 • FAX 800.437.2966

AliMed.com  
IFU-0013 ECO 1031  
©2021 AliMed® Inc. All rights reserved.  
#7968REV1121

# AliMed® Tilt Table Strap

## Instructions for Use and Care

### Intended Use

The AliMed® Tilt Table Strap supports a patient during diagnostic or surgical procedures using a tilt table.


### Instructions for Use

*For use by Clinician only.*

Reusable.

1. With hook material facing up, place strap over patient and under rail on each side of table (*Figure 1*).
2. Pull ends of straps over patient and toward center of table to desired tension (*Figure 2*).
  - 2.1 To fasten, press hook material firmly into loop surface.

*NOTE: It is recommended to use three straps per patient to provide both practitioner and patient with added level of security and comfort (Figure 3).*

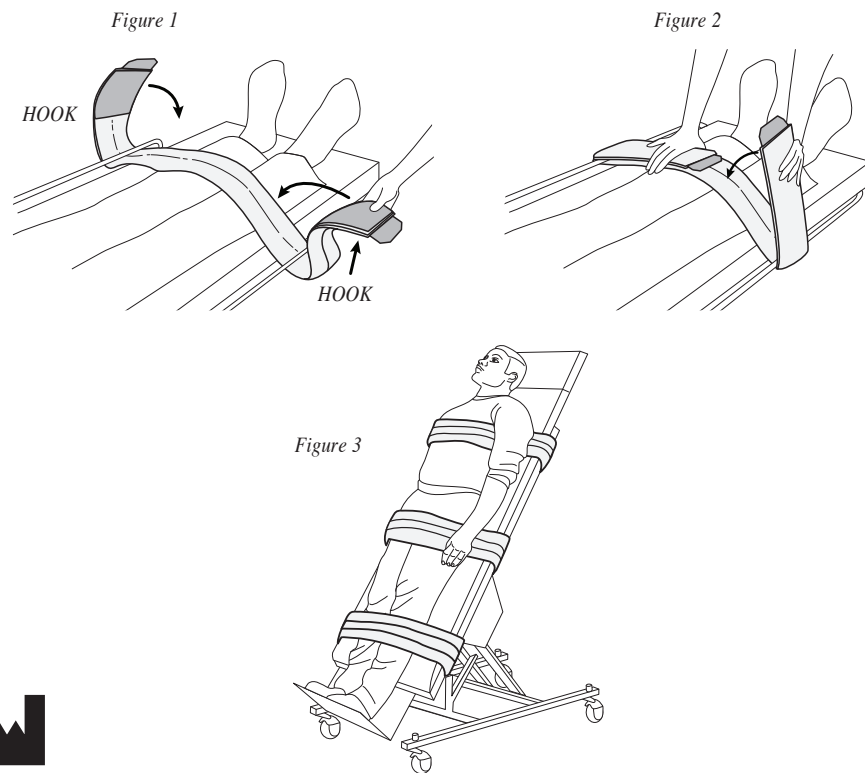

Manufactured for:



**AliMed® Inc.**

297 High St., Dedham, MA 02026 USA  
PH 800.225.2610 • FAX 800.437.2966

AliMed.com  
IFU-0013 ECO 1031  
©2021 AliMed® Inc. All rights reserved.  
#7968REV1121

### Contraindications/Warnings



- Do not use belt as a restraint.
- Allow to dry completely before use.
- Do not use strap if any part of hook or loop is compromised such that hook-and-loop closure does not fasten securely.
- Do not use if the patient has ever had an allergic reaction to any of the materials.
- Do not wrap strap circumferentially around table.
- Consult your institution's guidelines for assessing the risk of each individual patient.
- Report any serious incident to AliMed and the appropriate regulatory body.

### Care and Cleaning

May be cleaned with soap and water or standard machine washing and detergent. For machine washing, it is recommended that the hook-and-loop closure be securely fastened and the belt be placed in a cloth bag to prevent damage to the belt, or from the belt. For best results, let air dry.

### Materials



Strap: Nylon  
Not made with natural rubber latex.

### Storage/Disposal

Store in a clean, dry environment protected from direct sunlight. Storage at ambient room temperature is advised. Dispose of in accordance with existing federal, state, and local environmental control laws.

### Item Numbers



#7693

### Warranty

The ALIMED warrants to Purchaser that the Product(s) sold hereunder, is at the time of shipment to Purchaser from ALIMED, free from defects in material and workmanship. As Purchaser's sole exclusive remedy under this warranty ALIMED agrees either to repair or replace, at ALIMED's sole option and free of charge to Purchaser, any part or parts of such Product(s) which under proper and normal conditions of use prove to be defective within six months from the date of shipment. Visit [AliMed.com/terms](http://AliMed.com/terms) for full warranty info.



Manufactured for:



**AliMed® Inc.**

297 High St., Dedham, MA 02026 USA  
PH 800-225-2610 • FAX 800-437-2966

AliMed.com  
IFU-0013 ECO 1031  
©2021 AliMed® Inc. All rights reserved.  
#7968REV1121

### Contraindications/Warnings



- Do not use belt as a restraint.
- Allow to dry completely before use.
- Do not use strap if any part of hook or loop is compromised such that hook-and-loop closure does not fasten securely.
- Do not use if the patient has ever had an allergic reaction to any of the materials.
- Do not wrap strap circumferentially around table.
- Consult your institution's guidelines for assessing the risk of each individual patient.
- Report any serious incident to AliMed and the appropriate regulatory body.

### Care and Cleaning

May be cleaned with soap and water or standard machine washing and detergent. For machine washing, it is recommended that the hook-and-loop closure be securely fastened and the belt be placed in a cloth bag to prevent damage to the belt, or from the belt. For best results, let air dry.

### Materials



Strap: Nylon  
Not made with natural rubber latex.

### Storage/Disposal

Store in a clean, dry environment protected from direct sunlight. Storage at ambient room temperature is advised. Dispose of in accordance with existing federal, state, and local environmental control laws.

### Item Numbers



#7693

### Warranty

The ALIMED warrants to Purchaser that the Product(s) sold hereunder, is at the time of shipment to Purchaser from ALIMED, free from defects in material and workmanship. As Purchaser's sole exclusive remedy under this warranty ALIMED agrees either to repair or replace, at ALIMED's sole option and free of charge to Purchaser, any part or parts of such Product(s) which under proper and normal conditions of use prove to be defective within six months from the date of shipment. Visit [AliMed.com/terms](http://AliMed.com/terms) for full warranty info.



Manufactured for:



**AliMed® Inc.**

297 High St., Dedham, MA 02026 USA  
PH 800-225-2610 • FAX 800-437-2966

AliMed.com  
IFU-0013 ECO 1031  
©2021 AliMed® Inc. All rights reserved.  
#7968REV1121