

Care

1. Wipe with soft, non-abrasive cloth using a 1:10 bleach solution (contains 0.5% chlorine concentration) or follow your facility's cleaning protocol.
2. Do not immerse in fluids.
3. After cleaning, check unit is functioning properly.

Warning

Failure to comply with warning may result in injury or death. This device is not suitable for all individuals. Other devices may be required. This device is not a substitute for visual monitoring by caregiver. The manufacturer does not claim that this device will stop elopement and/or stop falls. It is a supplemental device to be used as part of a facility's overall fall management program. This product is to be used by a licensed caregiver only. As such, it is the entire responsibility of the caregiver to ensure that the system is properly installed and tested. Further, the system is not designed to replace good caregiving practices including, but not limited to:

- a.) Direct patient supervision
- b.) Adequate training for personnel for fall prevention and elopement
- c.) Testing of the system before each use

Report any serious incidents to AliMed and the appropriate regulatory body.

Limited Warranty: Seller warrants that the goods sold will be free from defects of workmanship and manufacturing for a period of one year from the date of sale.

Item Numbers

REF #713815

Environmental Conditions

| | Operational | Storage | Transport |
|-------------|---------------------------|--------------------------|--------------------------|
| Temperature | 10°–40°C 50°–104°F | -25°–70°C -13°–158°F | -25°–70°C -13°–158°F |
| Humidity | 30%–75% Non-condensing | 0%–95% Non-condensing | 0%–95% Non-condensing |
| Pressure | 700–1060 hPa | 700–1060 hPa | 700–1060 hPa |

CONFORMS TO AAMI STD ES60601-1, IEC STD 60601-1-6
CERTIFIED TO CSA STD C22.2 NO. 60601-1, NO. 60601-1-6

Symbol Glossary

| | |
|---|---|
|  | Manufacturer |
|  | Batch Code/Lot Number |
|  | Catalog Number/Item Number |
|  | Serial Number |
|  | European Conformity Mark |
|  | Authorized representative in the European Community |
|  | Tested/certification for compliance to published industry standards |
|  | Consult instructions for use |
|  | Caution: Read all warnings and precautions in instructions for use |
|  | DO NOT THROW IN TRASH |
|  | Indicates FCC has certified device |
|  | Indicates compliance to RoHS and is free of substances banned by RoHS |
|  | Do not re-use |
|  | Medical Device |

MDSS GmbH
Schiffgraben 41
30175 Hannover,
Germany



Manufactured for:



AliMed® Inc.

297 High St., Dedham, MA 02026 USA
PH 800.225.2610 • FAX 800.437.2966

AliMed.com

#7719REV0321 CCO1069

©2021 AliMed® Inc. All rights reserved.

Made in China



AliMed ONE® Wireless Alarm Base

Instructions for Use, Setup, and Care

Intended Use

The AliMed ONE Wireless Alarm Base is a central fall alarm unit that pairs with up to six compatible wireless fall monitoring devices (Hall Alert, Motion Sensor, Sensor Pad Transmitter) for caregiver notification of patient falls or elopement as part of an overall fall management program. The Alarm Base includes an integrated nurse call cable for connection with a nurse call system.

Key Features (External)

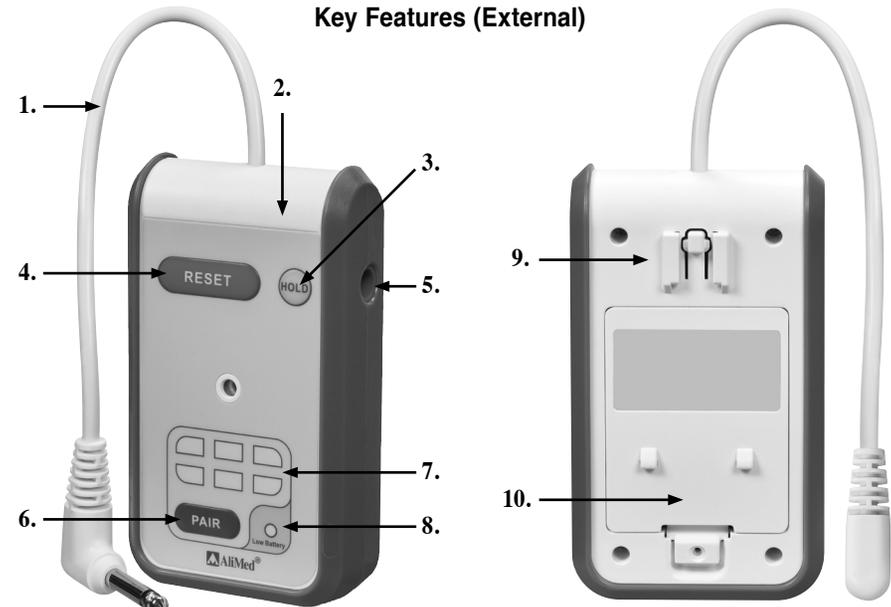


Figure 1

Figure 2

1. **Nurse Call Cable** Integrated 1-ft. (30.5-cm) cable connects with nurse call system
2. **Alarm Status Indicator** Illuminates when system status changes (Hold/Alarm)
3. **Hold Button** Places system on hold when moving patients
4. **Reset Button** Resets alarm system
5. **AC Adapter Input** Optional power source for use without batteries (120-240VAC, sold separately, see setup instructions)

6. **Pair Button** Pairs monitoring devices to Alarm Base
7. **Channel Status Indicator** Illuminates when monitoring device is paired
8. **Low Battery Indicator** Illuminates when battery is low and ready for replacement
9. **Universal Wall Mount** Holds bracket for mounting Alarm Base to wall
10. **Battery Compartment** Contains functional setting switches and battery compartments

Key Features (Internal)

- 1. Nurse Call Notification Setting**
Adaptable to different nurse call systems, three options: SP—Single Pulse, P—Pulse, C—Continuous
- 2. Volume Setting** Four options:
S—Silent, L—Low 80dB, M—Medium 90dB, H—100dB
- 3. Tone Setting** Three options: 1, 2, 3
- 4. Clear Channels Button** Clears all paired devices from Alarm Base memory
- 5. Lock/Pair Setting** Disables or enables the pairing function
- 6. Battery Compartment** Holds 3 AA batteries (not included)



Figure 3

Setup

The Alarm Base may be connected to the nurse call system (inside patient room) by Nurse or Biomedical staff. Set up unit based on nurse call requirement. *Note: Unit will operate without being connected to a nurse call system, however nurse call notifications will not be enabled.*

1. Alarm Base requires three (3) AA batteries to operate (not included). Optional AC Adapter can be used in place of batteries (sold separately, please contact your AliMed representative for ordering information).
2. Unscrew the battery compartment. Place screw in a safe place.
3. Lift battery compartment door by pulling handle upward.
4. Place batteries in the battery compartments according to configuration shown (Fig. 3). All LEDs on the unit will blink three (3) times accompanied by a beep.
5. Set preferences for Nurse Call Notification (SP, P, C), Volume (S, L, M, H), and Tone (1, 2, 3) by moving the appropriate switch left or right (Fig. 3). *Note: It is recommended to set the volume to Medium during setup/pairing to verify proper functionality. Once setup/pairing is complete, change the volume to desired setting.*
6. Press Clear Channels Button (Fig. 3). After a series of green blinking LEDs on the Alarm Status Indicator (Fig. 1), the first Channel Status Indicator (Fig. 1) will momentarily blink yellow, then all LEDs with blink three (3) times.
7. Alarm Base is now ready to pair with devices.
8. When setup is complete, close the battery compartment door and secure it with the screw.

Note: Change batteries when Low Battery Indicator illuminates (Fig. 1).

Operating Instructions

The Alarm Base allows pairing with up to six (6) compatible wireless monitoring devices:

- Hall Alert
- Motion Sensor
- Sensor Pad Transmitter (one required for each sensor pad)

Pairing the Alarm Base to a monitoring device:

1. Press Pair Button on Base (Fig. 1).
2. The Base will beep and the first open channel will blink green and red indicating channel is ready for pairing.
3. Place monitoring device next to the Base, matching PAIR on the device to PAIR on the Base (Fig. 4). *Note: PAIR/Pair Status Indicator on device will illuminate when in range.*
4. If pairing is successful, the Base will beep and the assigned channel will blink green once.
5. See individual instructions for each monitoring device for complete setup.

Match PAIR on device to PAIR on Base




Figure 4

Wall Mounting Instructions

1. Place metal part of bracket flat against Alarm Base (sticker side out).
2. Slide bracket upward until it locks securely in place (Fig. 5).
3. Peel film from adhesive stickers then press against wall to mount.
4. For additional security, it is also recommended to secure the bracket to the wall using the screws provided.
5. Connect nurse call cable to nurse call system. *Note: Unit will operate without being connected to a nurse call system, however nurse call notifications will not be enabled.*
6. The Alarm Base is now ready to use.

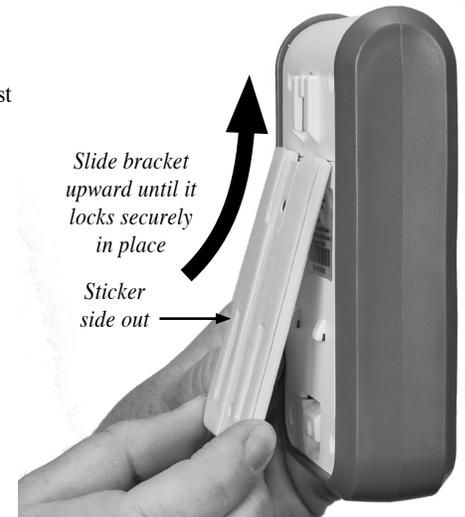


Figure 5